




Classic Longitudinal Wall-Mounted Exam Table

- *Stainless Steel Construction - Designed to Last*
- *Two-sided Work Surface*
- *Storage Drawer Accessible from Both Sides*
- *Raised Edge Minimizes Fluid Spills*

New Model Number: 12570-00-GZAADG
Former Model Number: 102590-00



SSCI

Wheeling, IL 800 323 7366

Table of Contents

General Information	3
Introduction	3
About this Manual	4
Conventions Used in this Manual	4
Notes	4
CAUTIONS	4
Available Accessories	4
Care and Cleaning of Stainless Steel	5
Introduction	5
Cleaning and Cleansers	5
Deodorizing Agents, Disinfectants, and Sanitizers	5
Effect on Warranty	6
Warranty	6
SSCI Contact Information	7
Parts Ordering Procedure	7
Returning the Table for Repairs	8
RMA Numbers	8
Packing and Shipment	8
Assembly & Installation	9
General	9
Pre-assembly Preparation	9
Assembly Procedures	9
Un-packing and Inspection	9
Parts Included	9
Tools and Supplies Required	10
Drilling the Mounting Holes	10
Mounting the Table to the Wall	12
Installation of Accessory Tie-down Brackets	13
Tools Required	14
Procedure	14
Cleaning	15
Introduction	15
Cleaning Procedures	15

© Copyright 2005 by **Suburban Surgical Co., Inc.** All rights reserved.

No part of this document may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying, recording, or by any information storage and retrieval system without written permission.

Inquiries should be addressed to **Suburban Surgical Co., Inc.**
Wheeling, Illinois 60090, USA

General Information



Introduction

SSCI's Classic Longitudinal Wall-Mounted Exam Table extends out from the wall to provide you with a two-sided work surface with plenty of leg room.

The rigid frame and stainless steel support bracket mount the table securely to the wall to give exam and treatment rooms a more open feeling while maximizing available work space.

A stainless steel backsplash prevents fluids and debris from being trapped between the wall and table, and a roomy storage drawer opens from either side for quick accessibility.

Edges are flanged down and hemmed to help eliminate sharp corners, and a Melamine finished undersurface repels moisture for easy care and long life. The table can be mounted at any convenient height to meet your needs.

About this Manual

Every attempt has been made to insure that the information in this manual is correct and complete. SSCI, however, always welcomes our customer's suggestions for improvements to our products and associated publications.

Conventions Used in this Manual

Throughout this manual you will find text under the headings **Note:** and **CAUTION:**.

Notes

Under the **Note:** heading, you will be given additional information pertinent to the subject discussed in that paragraph or procedural step.

Example:

Hold a single tie-down in place, and mark the centers of the three holes on the table side. **Note:** The single, center hole should go toward the bottom.

CAUTIONS

Under the **CAUTION:** heading, you will be alerted to potentially hazardous conditions which, if ignored or mishandled, could result in injury to yourself, or damage to the equipment.

Example:

CAUTION; Unpacking and assembling the exam table is not difficult. However, the table is heavy and we recommend that unpacking and assembly be done by at least two people.

Available Accessories

The following accessories increase the operating convenience of your Classic Exam Table. Find descriptions, pictures, and information on SSCI products and accessories in our current catalog, or on our website at www.suburbansurgical.com. To order accessories, refer to *Parts Ordering Procedure* on Page 7.

- Tie-down Brackets (set of 4) - P/N 12805-00-AAAAAA
- Black Vinyl Ribbed Mat - P/N 12800-00-GNAACV

Care and Cleaning of Stainless Steel

Introduction

Stainless steel is steel alloyed with chromium to make it highly resistant to stain, rust, and corrosion. **Note:** This does NOT mean that stainless steel will *never* rust or corrode. Science has not yet developed a steel which is completely stainless or corrosion PROOF.

The type of stainless steel and finish selected by SSCI for the table top is the best available for the intended use.

Cleaning and Cleansers

The basic rule of thumb is to use the mildest cleaning procedure that will do the job effectively. Always rinse thoroughly with clear water and dry completely. Frequent cleaning will prolong the service life of stainless steel equipment and will help maintain a bright, pleasing appearance.

Ordinary deposits of waste and fluids can usually be removed with soap and water. More stubborn deposits or tightly adhering debris may require harder scrubbing and possibly the use of commercial cleaning products acceptable for use on metal surfaces. When using any cleaning agent, rub in the direction of the polish lines or “grain” of the metal. For high luster finishes, clean soft cloths or pads should be used.

If especially rough cleaning is necessary, use “stainless steel” wool, nylon, or plastic scrubbers. Test these scrubbers in an inconspicuous area first to be sure they do not mar or scratch the stainless steel finish.

Minor scale build-up and some hard water spotting may be removed by washing with vinegar, followed by a neutralizing rinse with clear water and a thorough drying with a soft cloth. For heavy deposits of scale, 5% oxalic acid (use warm), 5-15% sulfamic acid, or 5-10% phosphoric acid may be used. Always follow with a neutralizing rinse of clean water and a thorough drying.

Deodorizing Agents, Disinfectants, and Sanitizers

The large selection of brands and combinations of chemicals available for deodorizing, disinfecting, and sanitizing is staggering. Select one or more agents for use in your facility only after weighing all the benefits claimed by each product. Often this choice is made without adequate consideration of the effects these agents may produce on equipment or furnishings.

CAUTION: Before selecting a chemical to employ in your facility, review label statements regarding use with metals (stainless steel). Always consult the chemical supplier if there are any doubts.

Avoid prolonged use of chlorides (such as chlorine bleach), bromides, iodides, and thiocyanates on stainless steel surfaces as these chemicals will cause pitting, corrosion, and metal discoloration. Allowing salty solutions to evaporate and dry on stainless steel may also contribute to corrosive conditions.

In summary, select chemical deodorizers, disinfectants, and/or sanitizers only after weighing all possible benefits and known adverse effects.

Effect on Warranty

CAUTION: The warranty for this product is void if the care and cleaning instructions provided in this manual are not followed.

Warranty

Suburban Surgical Company, Inc. warrants the original purchaser that our products are of the highest standards in material and workmanship. Our stainless steel components are guaranteed to last a lifetime assuming they are used as intended, properly maintained and cared for. Mechanical, electrical, electronic, hydraulic, and any product's devices carry a one year warranty.

Items purchased by Suburban Surgical Company, Inc. from other manufacturers and incorporated into our equipment are covered by the respective manufacturer's warranties.

Warranties will not apply if it is determined by Suburban Surgical Company, Inc. that the equipment became defective due to an accident, misuse, abuse, improper maintenance, or alteration. Warranty freight charges are covered for the first year only.

SSCI Contact Information

SSCI Customer Service can be contacted via mail, telephone, or fax. The department is available from 8:30am to 5:00pm, Central Time, Monday through Friday. Closed holidays.

Address: Suburban Surgical Co., Inc.
275 Twelfth Street
Wheeling, Illinois 60090

Telephone: Illinois - (847) 537-9320, ext. 3518
Toll Free - 1-800-323-7366

Fax: (847) 537-9061

Web: www.suburbansurgical.com

Parts Ordering Procedure

Order new equipment, accessories, and/or replacement parts directly through SSCI Customer Service. You can order by mail, telephone, or fax. Refer to *SSCI Contact Information* above for address, telephone, and fax numbers.

Information on products and accessories can be found in our current product catalog. Request a catalog free of charge through SSCI Customer Service.

When ordering, please provide the following:

- Your name
- Company name
- Company account number
- Your telephone number
- Shipping address
- Billing address (if different from shipping address)
- Names, part numbers, and quantities of items being ordered
- Credit card number and expiration date, or other payment information
- Preferred method of shipment
- Information on whether the items are required on a normal or urgent basis

Returning the Table for Repairs

RMA Numbers

If your exam table should require return to SSCI for repairs, discuss the problem with one of our Customer Service Representatives. Obtain an RMA number (Return Merchandise Authorization) from them before shipping the unit back. **Note:** Merchandise returned without an RMA number will not be accepted.

Packing and Shipment

If you were able to keep the exam table shipping carton and pallet, repack the table into the carton, and staple or tape the cover securely in place.

If the original shipping carton is not available, pack the table as best you can to protect it during shipment.

Ship documentation with the table including:

- Destination
- RMA Number
- Your name, company, and address
- Your telephone number
- A description of the reason for returning the table

Assembly & Installation

General

This section guides you in assembling and installing the SSCI Classic Longitudinal Wall-Mounted Exam Table. If you should require additional assistance, please feel free to call SSCI Customer Service at 1-800-323-7366.

Pre-assembly Preparation

On new construction, we recommend that, prior to finishing the wall to which this table will be mounted, you exactly determine where on the wall it will be located. Back up the mounting screw locations with 2" x 6"s. On an existing wall, you may want to open the wall and install these supports. These steps are not required for masonry walls.

Use lag screws for mounting into wood, or toggle bolts for mounting into block.

Assembly Procedures

CAUTION: Unpacking and assembling the exam table is not difficult. However, the table is heavy and we recommend that unpacking and assembly be done by at least two people. Follow the instructions carefully to prevent injury to yourself or damage to the table.

Un-packing and Inspection

If the shipping container appears damaged in any way, contact the shipping company immediately. Save all damaged packing materials to assist in proving liability for damage.

Carefully inspect your exam table top while you unpack it. If any damage is noted, or if parts appear to be missing, call SSCI Customer Service at 1-800-323-7366.

Parts Included

Three parts/assemblies are included in the shipment (Figure 1):

- Table Assembly with Drawer
- Diagonal Support
- Crossbrace

Note: Table-to-wall mounting hardware is not included

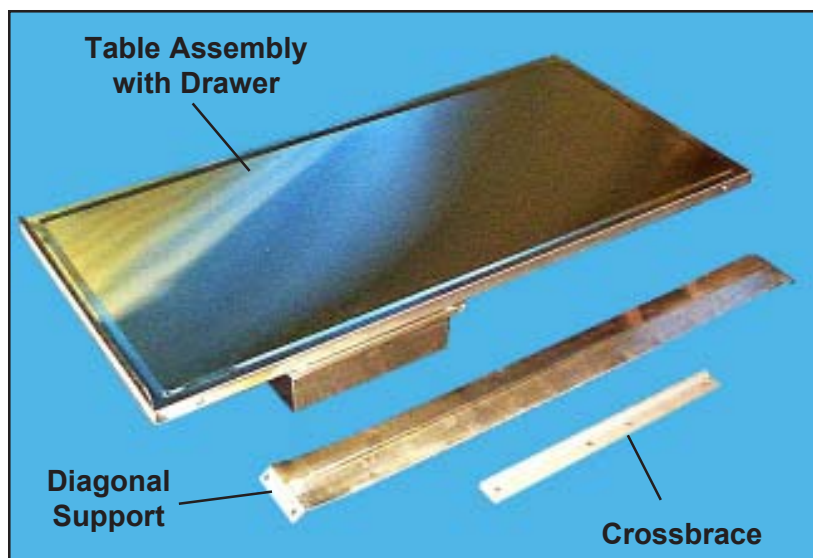


Figure 1. Parts Included with Wall-Mounted Exam Table

Tools and Supplies Required

You will need the following tools and supplies to install your wall-mounted table:

- Pen or pencil
- Tape measure
- Carpenter's Level
- Chalk line
- Power drill with appropriate size bits
- 1/2-in. wrench
- Mounting hardware suitable for wall
- Wrenches or screwdrivers for mounting hardware

Drilling the Mounting Holes

Locate and drill the seven mounting holes as follows. Refer to Figure 2 for dimensions. Select a drill bit size suitable for your selected mounting hardware. **Note:** The 35-in. height shown in Figure 2 is our recommendation. You can mount the table higher or lower if it is more convenient for you.

1. Locate two wall studs, 16-in. apart, in your selected table position.
2. Using a level, mark a horizontal line between these two studs, 35-in. above the floor (or other height, if preferred).
3. Find and mark two hole locations on this horizontal line, 16-in. apart, located so as to enter the centers of the studs.

4. Drill these two holes into the studs.
5. Find and mark the center point between these two holes (8-in. from either hole).
6. Drill a third hole at this center point.
7. From this center point, scribe a line down, vertically, 22-in. from the top holes, and mark a point.
8. From this point, mark a horizontal line at least 16-in. long on each side of the center line.
9. Locate four holes on this line:
 - Two holes 1-1/2-in. on either side of the vertical line. (These holes will then be 3-in. apart)
 - Two holes 8-in. on either side of the vertical line. (These holes will then be 16-in. apart)
10. Drill these four holes.

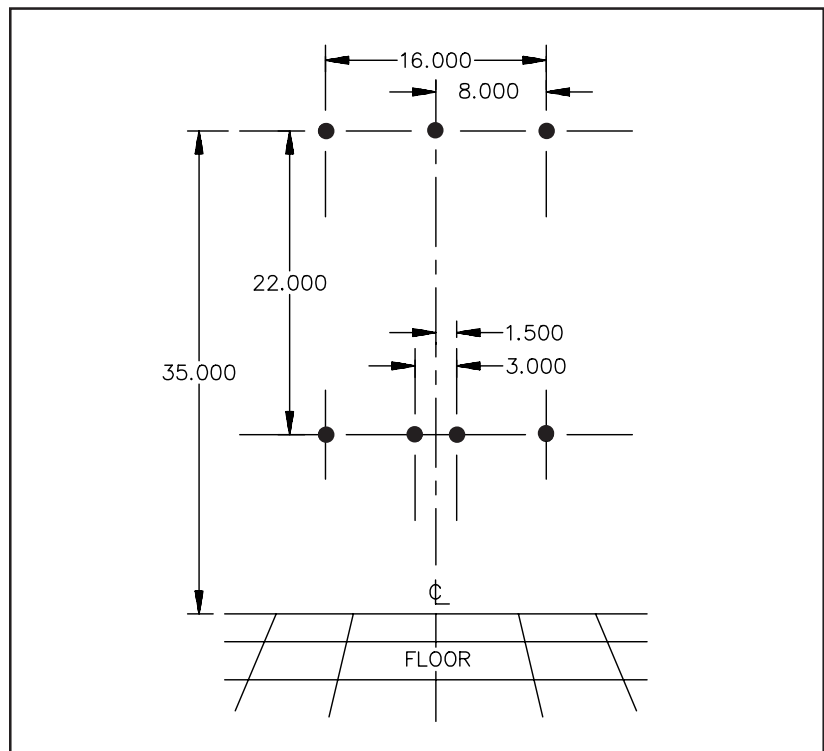


Figure 2. Mounting Dimensions

Mounting the Table to the Wall

Mount the table to the wall as follows. Refer to Figure 4.

CAUTION: Mounting the exam table to the wall is not difficult. However, the table is heavy and mounting it is very awkward for one person. We recommend that mounting be done by at least two people. Follow the instructions carefully to prevent injury to yourself or damage to the table.

1. On the underside of the table, with a 1/2-in. wrench, remove the two nuts and washers from the diagonal support mounting studs (Figure 3).

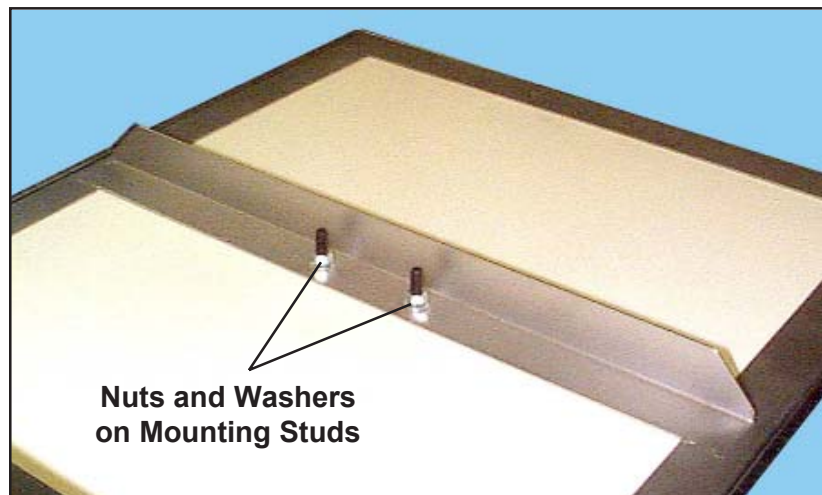


Figure 3. Nuts and Washers to be Removed

2. Mount the crossbrace to wall with screws or bolts through the lower, outer mounting holes (Figure 4).
3. Mount the diagonal support to the mounting studs on the underside of the table using the nuts and washers removed in *Step 1*.
4. Mount the table to the wall with screws or bolts through the upper three holes.
5. Mount the diagonal support to the crossbrace and wall with screws or bolts through the lower, inner mounting holes.

Installation of your new SSCI Longitudinal Wall-Mounted Exam Table is now complete.

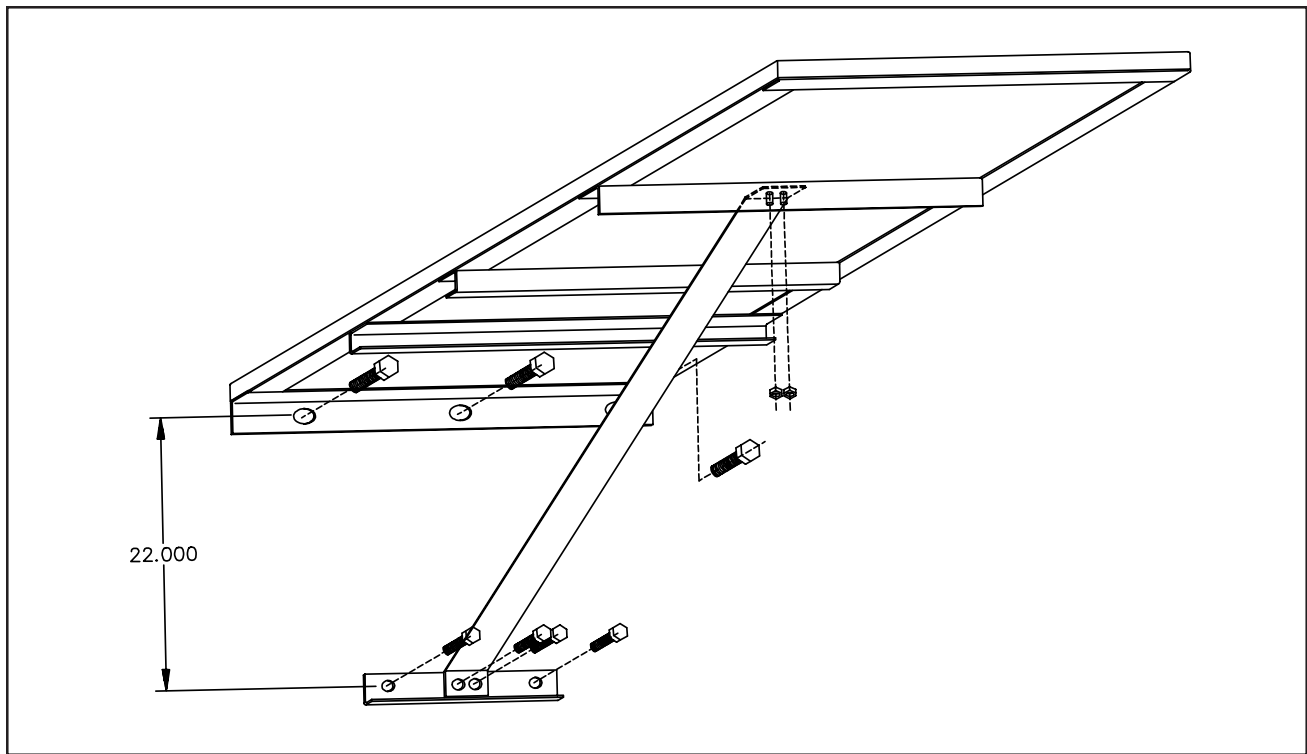


Figure 4. Installation of Table to the Wall

Installation of Accessory Tie-down Brackets

A set of tie-down brackets is available for use with your exam table. Order P/N 12805-00-AAAAAA. The set includes four tie-down brackets and 12 Phillips-head, self-tapping screws (Figure 5). To install these tie-downs, follow the steps below.

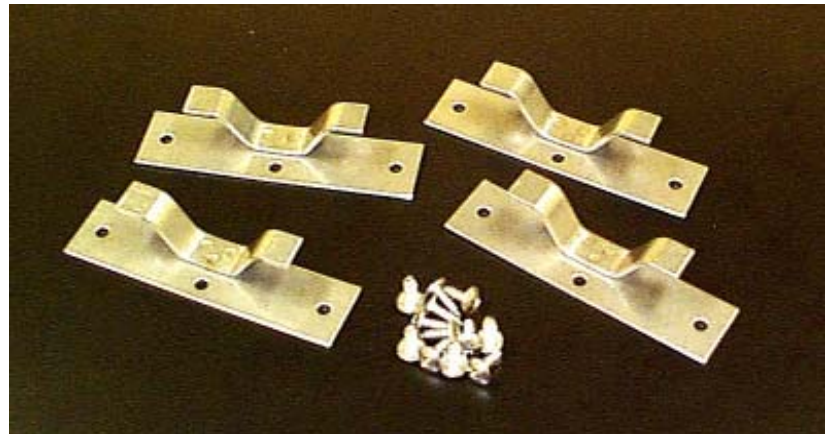


Figure 5. Tie-down Bracket Kit Contents

Two tie-downs should be installed to each side of the table.

Note: The tie-downs mount to the *edge* of the table, not the top. The locations of the tie-downs depend on the size of the animals to be examined. For smaller animals, the tie-downs should be installed close to the center of the table. For larger animals, the tie-downs should be installed farther apart, closer to the ends of the table.

Tools Required

- Tape measure or ruler
- Marking tool (pencil, pen, felt tip, etc.)
- Punch
- Hammer
- Electric drill
- 3/32-in. drill bit
- Phillips head screwdriver (or drive for electric drill)

Procedure

1. Determine where on the exam table you want the tie-downs installed. **Note:** Avoid placing the brackets over the existing screw heads in the side of the table.
2. Hold a single tie-down in place (Figure 6), and mark the centers of the three holes on the table edge. The single, center hole should be on the bottom.

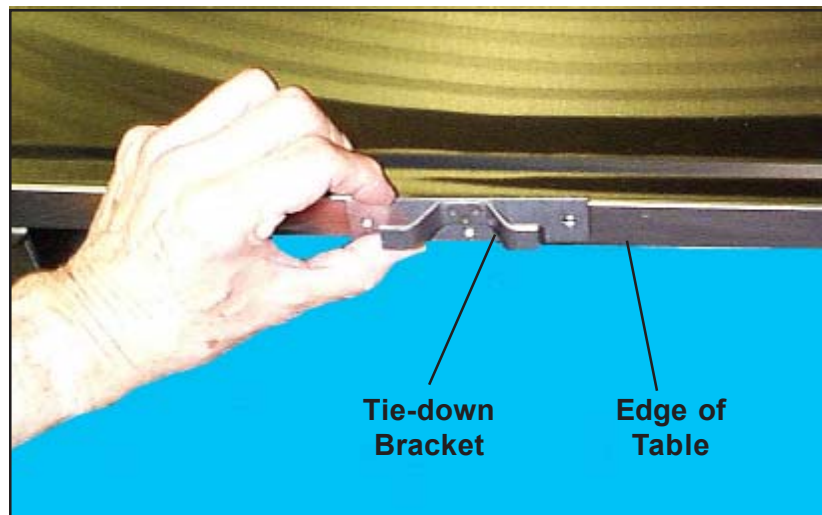


Figure 6. Holding Tie-down Bracket to Table Edge

3. With a punch and hammer, tap a small dimple in the metal at each of the hole center marks. These dimples serve as guides for the drill.
4. Drill the three holes with a 3/32-in. drill bit.
5. Mount the tie-down to the table with three of the screws provided in the kit.
6. Mount the remaining three tie-downs the same way.

Cleaning

Introduction

You will no doubt want to clean your exam table whenever it becomes dirty or saturated with waste fluids. Maintaining high standards of sanitation will be an important priority for your facility.

Cleaning Procedures

Whenever necessary, rinse the table with clear water and dry thoroughly with clean, soft cloths.

Ordinary deposits of waste and fluids can usually be removed with soap and water. Stubborn deposits may require scrubbing with “stainless steel” wool, nylon, or plastic scrubbers and/or the use of commercial cleaning products. Always scrub in the direction of the “grain” of the metal. Rinse with clear water and dry thoroughly with clean, soft cloths.


Minor scale build-up and some hard water spotting may be removed by washing with vinegar, followed by a neutralizing rinse of clear water and a thorough drying with clean, soft cloths.

For heavy deposits of scale, 5% oxalic acid (use warm), 5-15% sulfamic acid, or 5-10% phosphoric acid may be used. As always, rinse with clear water and dry thoroughly with clean soft cloths.

Avoid prolonged use of chlorides (such as chlorine bleach), bromides, iodides, and thiocyanates. Never allow salty solutions to dry on the stainless steel.

CAUTION: The warranty for this product is void if the care and cleaning instructions provided in this manual are not followed.

For more information on SSCI's fine line of products and accessories, talk to your SSCI sales representative.



Suburban Surgical Company, Inc.
275 Twelfth Street **Wheeling, IL 60090**
Phone: (847) 537-9320 Fax: (847) 537-9061
Toll Free: 1-800-323-7366 Web: www.suburbansurgical.com