




Imperial 6 Laminated Prep-Procedure Table

- *Top quality laminated construction for durability*
- *Variety of widths and styles to suit your needs*
- *Cabinet-style for beauty and efficiency*
- *Stainless steel tub & removable prep rack*

Model Numbers: Vary with widths and styles - refer to SSCI catalog



SSCI

Wheeling, IL (800) 323 7366

Table of Contents

Chapter 1 - General Information	5
Introduction	5
About this Manual	6
Information and Safety Notices	6
Notes	6
CAUTIONS	6
SSCI Contact Information	6
Models	7
Accessories	7
Care and Cleaning of Stainless Steel	7
Introduction	7
Cleaning and Cleansers	7
Deodorizing Agents, Disinfectants, and Sanitizers	8
Effect on Warranty	8
Cleaning Requirements	9
Warranty	9
Chapter 2 - Installation	10
General	11
Unpacking and Inspection	11
Preparation	11
Installation Procedure	11
Overview	11
Tools and Supplies Required	11
Installation Sequence	12
Determine the Table Location	12
Open the Wall or Floor	12
Install the Piping for the Faucet and Drain	12
Open Holes in the Table Wall/Floor	12
Finish the Room Wall or Floor	13
Place the Table in Position	13
Connect the Drain	13
Install the Faucets	13
Finish the Job	13
Disposition of the Shipping Carton	13

© Copyright 2006 by **Suburban Surgical Co., Inc.** All rights reserved.

No part of this document may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying, recording, or by any information storage and retrieval system without written permission.

Inquiries should be addressed to **Suburban Surgical Co., Inc.**

Wheeling, Illinois 60090, USA

Chapter 3 - Use and Care	14
Using Your Prep-Procedure Table	15
Using the Drawers	15
Opening and Closing the Drawers	15
Removing and Replacing a Drawer	15
Using the Doors	16
Opening and Closing the Doors	16
Hinges - Overview	16
Removing a Door	16
Installing a Door	17
Adjusting the Door Left-to-Right	17
Adjusting the Door In-and-Out	18
Using Prep-Procedure Racks	19
Overview	19
Removing and Installing a Rack	19
Keeping Your Imperial Prep-Procedure Table Clean	20
Introduction	20
Cleaning Laminated Surfaces	20
Sharp Objects	20
Dusting	20
Cleaning Tips	20
Substances to Avoid	20
Recommended Cleaners	21
Cleaners to Avoid	22
Cleaning Stainless Steel Tubs	22
 Chapter 4 - Parts Replacement.....	 22
Replacement Parts	23
General Information	24
Parts Ordering Procedure	24
Returning the Prep-Procedure Table for Repairs	24
RMA Numbers	24
Packing and Shipment	24
Parts Replacement Procedures	25
Door, Hinged Left or Hinged Right	25
Overview	25
Tool Required	25
Procedure	25
Door Hinge	26
Overview	26
Tool Required	26
Procedure	26
Door Hinge Mounting Plate	27
Overview	27
Tool Required	27
Procedure	27

Door Hinge <i>Suburban Surgical</i> Logo Cap	28
Overview	28
Procedure	28
Drawer	29
Overview	29
Procedure	29
Drop-in Tub	30
Overview	30
Tools Required	30
Procedure	30
Prep-Procedure Rack	31
Overview	31
Procedure	31
Removable Bathing Rack (Optional)	32
Overview	32
Procedure	32

Chapter 1 - General

Introduction



SSCI's Imperial 6 Prep-Procedure Table panels are made of 45 lb industrial-grade substrate, shaped on a CNC machine for accuracy, then dadoed and rabbeted to ensure tight fitting joints. All joints are glued with an adhesive impervious to liquids, and mechanically fastened to guarantee a solid, sturdy cabinet. All cabinet interiors are finished with Thermo-Fused Melamine, making them water, odor, and chemical-resistant. All finished, exterior surfaces including the body, drawer, and door edges are covered with high-pressure plastic laminate. Laminates are available in SSCI standard or optional colors, or you can choose from a spectrum of customer-selected colors to blend with your facility's decor.

The particleboard substrate used by SSCI for its laminates is the ideal solution for interior applications where high humidity and intermittent water contact are common, and is far more resistant to moisture and water exposure than conventional industrial particleboard. SSCI's particleboard is manufactured with highly compressed wood fibers and a specially formulated resin to produce a substrate with superior strength, rigidity, and an extra hard surface. Screw holding strength is substantially greater than typical industrial particleboard, while swelling caused by water soaking is much less.

Drawer backs and bottoms are .625 in. thick, and all drawers open and close easily even with heavy loads.

The door's positive-action, invisible hinges have self-closing mechanisms and 3D micro-adjustment. All door and drawer fronts have full-width aluminum pulls.

The tables covered in this manual are all top quality laminate construction, with nominal six inch deep drop-in tubs, and any of a wide selection of drawers and/or doors.

About this Manual

Every attempt has been made to insure that the information in this manual is correct and complete. SSCI, however, always welcomes our customer's suggestions for improvements to our products and associated publications.

Information and Safety Notices

In this manual you will find text under the headings **Note:**, and **CAUTION:**.

Notes

Under **Note:** headings, you will be given additional information pertinent to the subject discussed in that paragraph or step.

Example:

To install a rack, merely set it in place on the table.

Note: If the rack does not seem to fit, rotate it 180° and try again.

CAUTIONS

Under **CAUTION:** headings, you will be alerted to potentially hazardous conditions which, if ignored or mishandled, could result in injury to yourself or damage to the equipment.

Example:

CAUTION: Unpacking and installing the table is not difficult. The table is heavy, however, and handling it can be awkward for one person. We recommend that unpacking and installation be done by at least two people.

SSCI Contact Information

Contact SSCI Customer Service by mail, telephone, or fax. The department is available from 8:30am to 5:00pm, Central Time, Monday through Friday. Closed holidays.

Address: Suburban Surgical Co., Inc.
275 Twelfth Street
Wheeling, Illinois 60090

Telephone: Illinois - (847) 537-9320, ext. 3518
Toll Free - (800) 323-7366

Fax: (847) 537-9061

Web: www.suburbansurgical.com

Models

This *Owner's Manual* covers SSCI Imperial 6 laminated, cabinet-style prep-procedure tables. SSCI's cabinet prep-procedure tables, however, come in a wide variety of styles to enable you to custom-design the perfect table for your facility. The following options are available:

- Imperial laminated tables or Regal stainless steel tables
- Full-cabinet styles as well as cabinets with knee-space, middle, left, or right
- A wide range of drawer and/or door arrangements
- 48 in. or 60 in. wide cabinets
- Island or abutted styles
- Selection of faucets

Find descriptions, pictures, and part numbers for SSCI products and accessories in our current catalog, or visit our website at www.suburbansurgical.com. To order products, parts, or accessories, refer to *Parts Ordering Procedure* on Page 24.

Accessories

A variety of accessories is available for SSCI Imperial Prep-Procedure Tables to increase your convenience and efficiency. Refer to your current SSCI catalog for pictures, descriptions, and part numbers.

- Corner Edge Protectors
- Pull-out Trays
- "V" Prep-Procedure Racks
- Flat Prep-Procedure Racks
- Solid Removable Tops
- Tub Floor Removable Bathing Racks

Care and Cleaning of Stainless Steel

Introduction

Stainless steel is steel alloyed with chromium to make it highly resistant to stain, rust, and corrosion. **Note:** This does NOT mean that stainless steel will *never* rust or corrode. Science has not yet developed a steel which is completely stainless or corrosion PROOF.

The type of stainless steel and finish selected by SSCI for this product is the best available for the intended use.

Cleaning and Cleansers

The basic rule of thumb is to use the mildest cleaning agent that will do the job effectively. After cleaning, always rinse thoroughly with clear water, and dry completely. Frequent cleaning will prolong the service life of stainless steel equipment and will help maintain a bright, pleasing appearance.

Ordinary deposits of waste and fluids can usually be removed with soap and water. More stubborn deposits or tightly adhering debris may require harder scrubbing and possibly the use of commercial cleaning products acceptable for use on metal surfaces. When using any cleaning agent, rub in the direction of the polish lines or "grain" of the metal. For high luster finishes, clean soft cloths or pads should be used.

If especially rough cleaning is necessary, use "stainless steel" wool, nylon, or plastic scrubbers. Test these scrubbers in an inconspicuous area first to be sure they do not mar or scratch the stainless steel finish.

Minor scale build-up and some hard water spotting may be removed by washing with vinegar, followed by a neutralizing rinse with clear water, and a thorough drying with a soft cloth. For heavy deposits of scale, 5% oxalic acid (use warm), 5-15% sulfamic acid, or 5-10% phosphoric acid may be used. Always follow with a neutralizing rinse of clean water and a thorough drying.

Deodorizing Agents, Disinfectants, and Sanitizers

The large selection of brands and combinations of chemicals available for deodorizing, disinfecting, and sanitizing is staggering. Select one or more agents for use in your facility only after weighing all the benefits claimed by each product. Often this choice is made without adequate consideration of the effects these agents may produce on equipment or furnishings.

CAUTION: Before selecting a chemical to employ in your facility, review label statements regarding use with metals (stainless steel). Always consult the chemical supplier if there are any doubts.

Avoid prolonged use of chlorides (such as chlorine bleach), bromides, iodides, and thiocyanates on stainless steel surfaces as these chemicals will cause pitting, corrosion, and metal discoloration. Allowing salty solutions to evaporate and dry on stainless steel may also contribute to corrosive conditions.

In summary, select chemical deodorizers, disinfectants, and/or sanitizers only after weighing all possible benefits and known adverse effects.

Effect on Warranty

The warranty for this product is void if the care and cleaning instructions provided in this manual are not followed.

Cleaning Requirements

Clean the prep-procedure table exactly in accordance with the cleaning instructions provided in Chapter 3 of this manual.
Failure to follow these instructions can void your warranty.

Warranty

Suburban Surgical Company, Inc. warrants the original purchaser that our products are of the highest standards in material and workmanship. Our stainless steel components are guaranteed to last a lifetime assuming they are used as intended, properly maintained and cared for. Mechanical, electrical, electronic, hydraulic, and any product's devices carry a one year warranty.

Items purchased by Suburban Surgical Company, Inc. from other manufacturers and incorporated into our equipment are covered by the respective manufacturer's warranties.

Warranties will not apply if it is determined by Suburban Surgical Company, Inc. that the equipment became defective due to an accident, misuse, abuse, improper maintenance or alteration. Warranty freight charges are covered for the first year only.

Chapter 2 - Installation

General

This section guides you in unpacking, inspecting, and installing the SSCI Imperial 6 Laminated Prep-Procedure Table. If you have problems or require additional assistance, please call SSCI Customer Service at (800) 323-7366.

Unpacking and Inspection

CAUTION: Unpacking the Imperial Prep-Procedure Table is not difficult. The table is heavy, however, and we recommend that unpacking be done by at least two people.

If the shipping container appears damaged in any way, contact the shipping company immediately. Save all damaged packing materials to assist in proving liability for damage.

Carefully inspect the table as you unpack it. If any damage is noted, or if parts appear to be missing, call SSCI Customer Service at (800) 323-7366.

Preparation

The Imperial 6 Prep-Procedure Table comes fully assembled. The only work required is the installation of the faucets and connection to the water supply and drain. SSCI recommends a thorough cleaning before placing the table in service. Please read this *Owner's Manual* before using the table, and then safely file the manual where it can be quickly accessed for future reference.

Installation Procedure

Overview

The following instructions give you a general plan for installing the prep-procedure table. Since every installation will be unique, it is obviously impractical to specify exact instructions for every case. A photo may show a knee-space left or knee-space right table, however, knee-space left and right tables are exact mirror-images of each other.

Tools and Supplies Required

You will need the following tools and supplies to install your prep-procedure table.

- Plumbing tools and supplies as needed
- Electric drill and hole cutters of required sizes

Installation Sequence

We suggest the following installation sequence:

1. Determine the table location.
2. Open the wall or floor (if necessary to pipe in the faucet and drain - may not be required on new construction).
3. Install the piping for the faucet and drain.
4. Open holes in the table wall/floor as necessary.
5. Finish the room wall or floor.
6. Place the table in position.
7. Connect the drain.
8. Install the faucets.
9. Finish the job.

Determine the Table Location

Determine exactly where you want the prep-procedure table to be installed. Among other requirements, the location should provide efficient, convenient, and cost-effective routing for the faucet and drain plumbing.

Open the Wall or Floor

If this is not new construction, open the wall or floor as necessary to install piping for the prep-procedure table faucets and drain.

Install the Piping for the Faucet and Drain

Install the piping as necessary for the table faucets and drain. Use only deck-mounted faucets; the prep-procedure table is not designed for use with wall-mounted faucets.

Open Holes in the Table Wall/Floor

Plumbing can be brought into the table from the rear, side, or the floor, depending on the location of the table and the layout of the room. Locate and open holes as necessary in the rear wall, side wall, or floor of the prep-procedure table (Figure 1) as necessary to allow entrance of the drain and water piping.

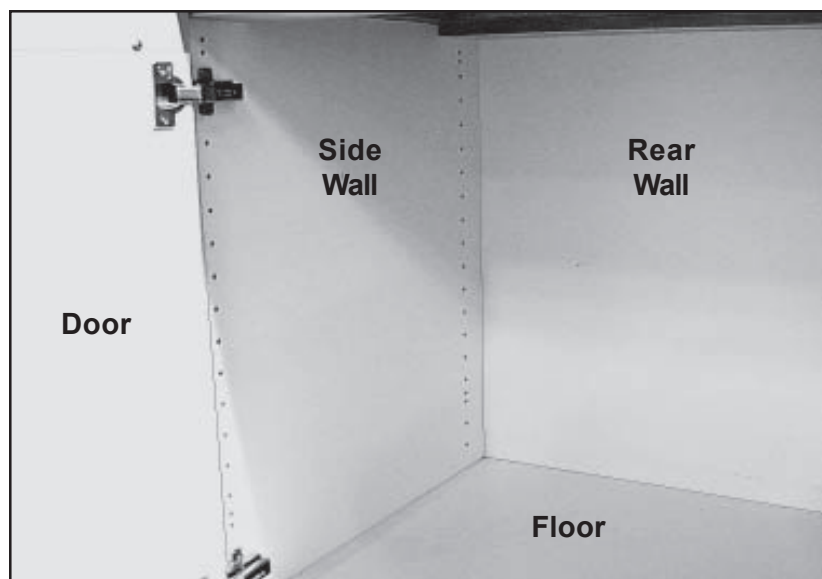


Figure 1. Interior View of Typical Prep-Procedure Table

**Finish the Room
Wall or Floor**

After plumbing is complete, the room wall and or floor can be finished.

**Place the Table
in Position**

Put the table in its intended position.

Connect the Drain

Connect the drain piping to the tub drain (Figure 2).

Install the Faucets

1. Install and connect the faucets according to the instructions enclosed with the units (Figure 2).
2. Run water into the prep-procedure table and make sure the plumbing is correct and free of leaks.

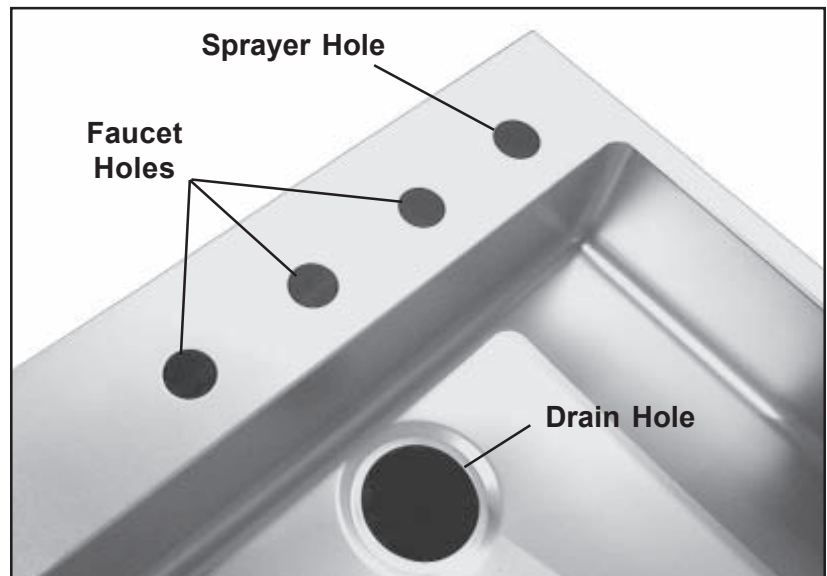


Figure 2. Faucet, Sprayer, and Drain Locations

Finish the Job

1. Place the basket strainer into the drain opening.
2. Place a prep rack on the table, if desired.

**Disposition of the
Shipping Carton**

The shipping carton can be cut up and thrown away. If adequate storage space is available, however, it might be handy to retain the carton in case reshipment of the table to the manufacturer for repairs ever becomes necessary.

Chapter 3 - Use and Care

Using Your Prep-Procedure Table

Using the Drawers

Opening and Closing the Drawers

The following instructions apply to both three and four drawer tables. The drawers on the Imperial Prep-Procedure Table are designed to work smoothly even with heavy loads.

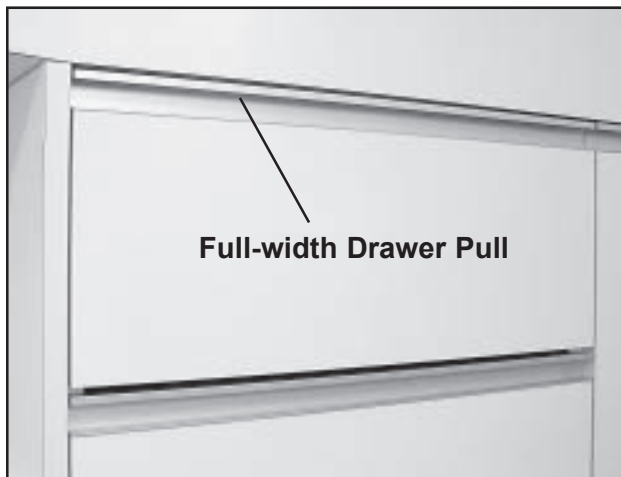


Figure 3. Full-width Drawer Pull

To open a drawer, turn your palm upward and, with your fingertips, grasp the full-width pull (Figure 3), then gently pull the drawer open.

To close the drawer, gently push the drawer in. Avoid overfilling the drawers so that the contents obstruct the movement of the drawers.

Removing and Replacing a Drawer

To remove a drawer, pull the drawer out, then tilt the front of the drawer up, and pull the drawer out of the cabinet.

To replace a drawer, slide the rollers at the rear of the drawer (Figure 4) over the rollers on the cabinet walls (Figure 5), then gently push the drawer in.

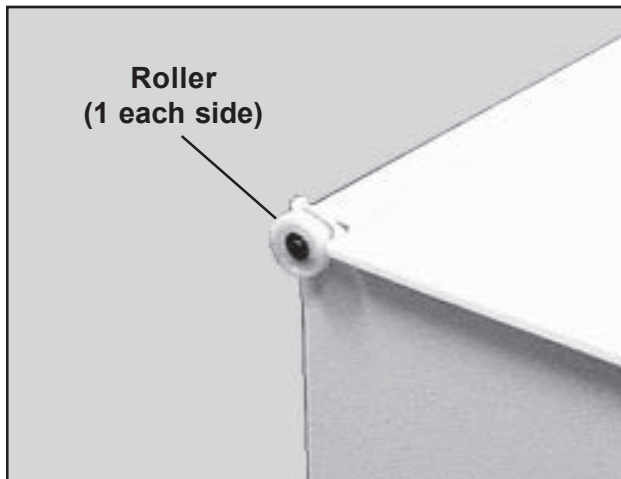


Figure 4. Roller on Rear of Drawer.

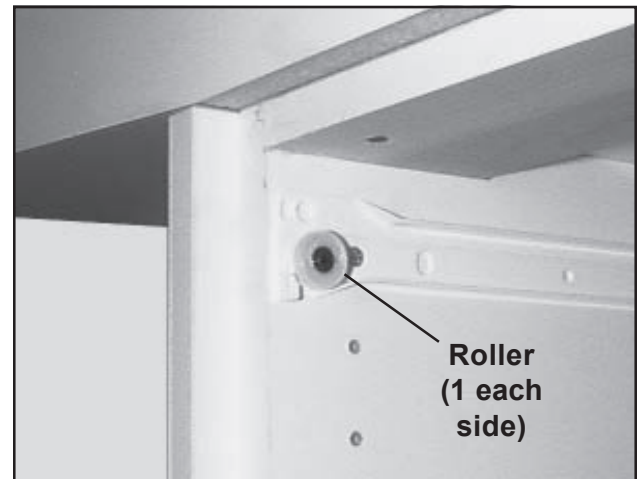


Figure 5. Roller on Cabinet Wall

Using the Doors **Opening and Closing the Doors**

The doors on the Imperial Prep-Procedure Table open approx. 110° for full and easy access to the interior. To open a door, turn your palm upward and, with your fingertips grasp the full-width pull (Figure 6), and gently pull the door open. The door will hold itself open. To close the door, gently push the door closed and the door will stay closed. The doors feature positive-action invisible hinges, and 3D micro-adjustment ensures correct door alignment.

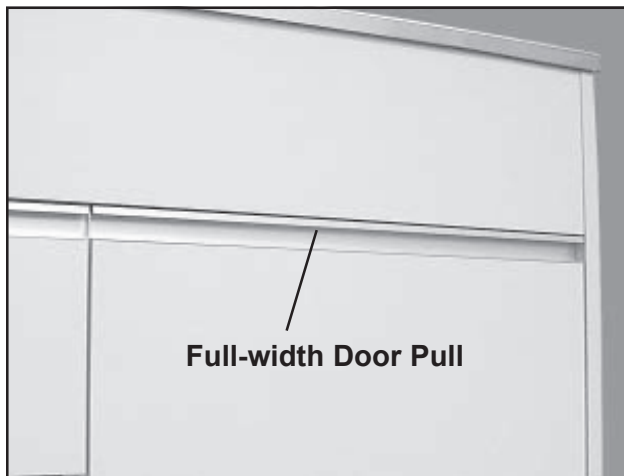


Figure 6. Full-width Door Pull

Hinges - Overview

The hinges used on the doors are sturdy, high quality devices. The following paragraphs will be helpful when removing or installing a door, or when adjusting the fit of a door in the cabinet. Figures 7 and 8 show close-up images of unmounted hinges to give you detailed views which would be difficult to obtain with the hinges mounted in place.

Removing a Door

The design of the hinges makes it easy to remove a door from the cabinet. To remove a door, squeeze the release catch on the hinge (Figure 7) and the hinge releases from the hinge mounting plate. When both hinges are released, the door comes off the cabinet.

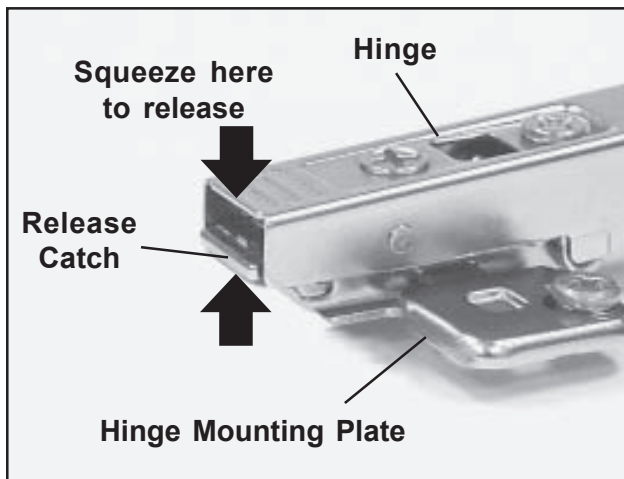


Figure 7. Hinge and Hinge Mounting Plate (unmounted)

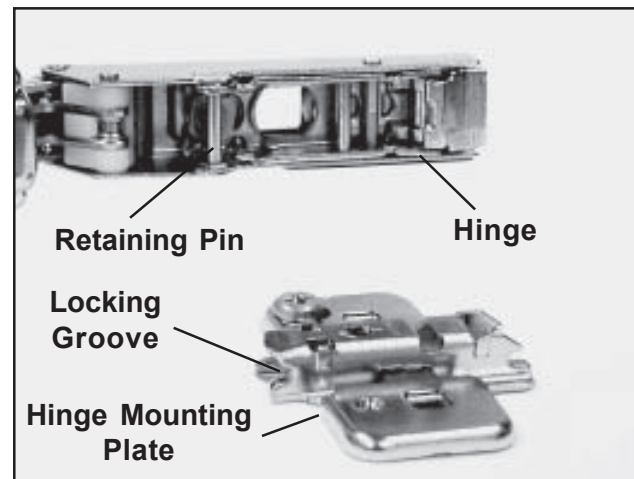


Figure 8. Hinge and Hinge Mounting Plate Separated

Installing a Door

Two hinges must be mounted to the door and two hinge mounting plates to the cabinet. Hook the retaining pin on the hinge into the locking groove in the hinge mounting plate (Figure 8). Then, pivot the hinge closed and press the end of the hinge down until it snaps into place. Do the same to both hinges to secure the door to the cabinet.

Adjusting the Door Left-to-Right

An adjustment on the hinge moves the door left and right within the door frame. By adjusting both hinges, you can center the door to provide equal spacing on the left and right. The door must be mounted on the cabinet to make this adjustment.

Tool Required: Phillips screwdriver

Procedure:

1. Close the cabinet door.
2. Observe the gaps between the left and right sides of the door and the door frame (Figure 9).
3. Open the door.
4. Pull the *Suburban Surgical* logo cap off the hinge.
5. With a Phillips screwdriver, turn the left-right adjustment screw (Figure 10) clockwise to move the door to the right; counterclockwise to move the door to the left.
6. Close the door and check the gaps.
7. Open the door and repeat the adjustment if necessary.
8. Continue as above until the gaps are equal.
9. Snap the *Suburban Surgical* logo cap back on the hinge.
10. Repeat the procedure for the other hinge.

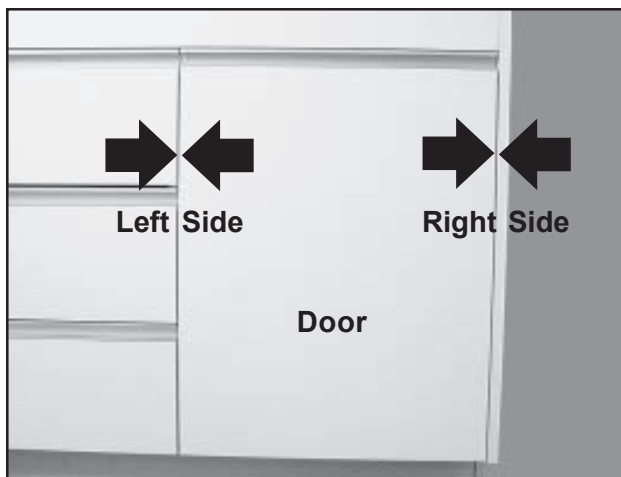


Figure 9. Adjusting the Door Left-Right



Figure 10. Door Left-Right Adjustment Screw

Adjusting the Door In-and-Out

An adjustment on the hinge moves the door in and out in the door frame. By adjusting both hinges, you can make the hinge side of the door flush with the cabinet frame. The door must be mounted on the cabinet to make this adjustment.

Tool Required: Phillips screwdriver

Procedure:

1. Close the cabinet door.
2. Observe whether or not the hinge side of the door is flush with the cabinet frame (Figure 11).
3. Open the door.
4. Pull the *Suburban Surgical* logo cap off the hinge.
5. With a Phillips screwdriver, turn the in-out adjustment screw (Figure 12) clockwise to move the door in; counterclockwise to move the door out.
6. Close the door and check to see if the door is flush with the cabinet frame.
7. Open the door and repeat the adjustment if necessary.
8. Continue as above until the door is flush with the frame.
9. Snap the *Suburban Surgical* logo cap back on the hinge.
10. Repeat the procedure for the other hinge.



Figure 11. Adjusting the Door In-Out

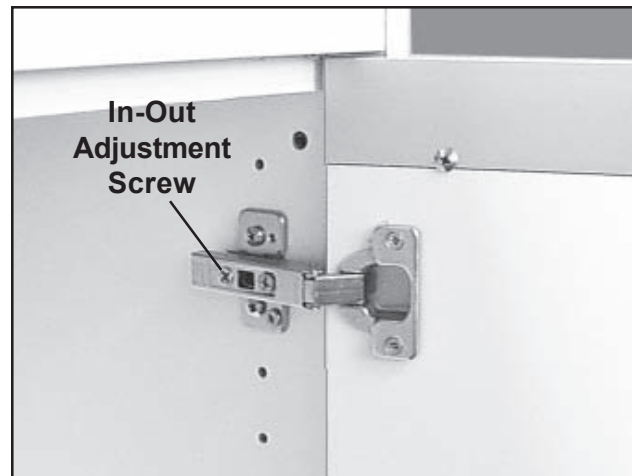


Figure 12. Door In-Out Adjustment Screw

Using Prep-Procedure Racks

Overview

Several styles of prep-procedure racks are available for use with the table. The racks are all easily removable without tools for cleaning or other activities. The available racks are:

- Flat prep-procedure rack
- “V” prep-procedure rack
- Extension rack for faucet area
- Solid removable top

Removing and Installing a Rack

CAUTION: Removing and installing a rack is not difficult. The rack is heavy, however, and handling it can be awkward for one person. We recommend that removal and installation of a rack be done by at least two people.

To remove a rack, simply pick it up by hand and lift it off the table. To install a rack, merely set it in place on the table. **Note:** If the rack does not seem to fit, rotate it 180° and try again.

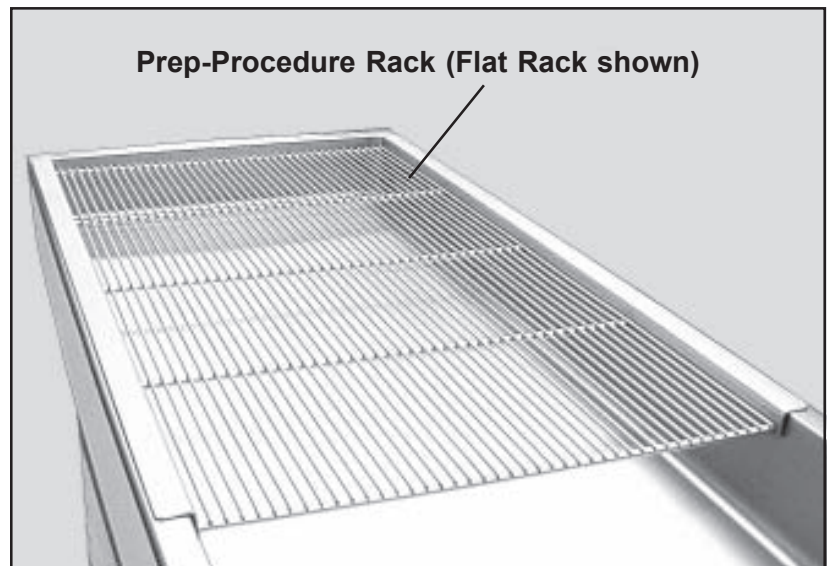


Figure 13. Prep-Procedure Rack

Keeping Your Imperial Prep-Procedure Table Clean

Introduction

You will no doubt want to clean your prep-procedure table frequently. Maintaining high standards of sanitation will be an important priority for your facility.

CAUTION: The warranty for this product is void if the care and cleaning instructions provided here are not followed.

Cleaning Laminated Surfaces

Sharp Objects

Sharp objects can damage the laminate surface, marring its beauty, and lowering wear and stain resistance. Although high pressure laminates are somewhat resistant to scratching and marring, the surface can be damaged even under normal use.

Dusting

The laminate may need occasional dusting. To keep the surface beautiful, use a non-oily furniture spray. (Remember to clean the spray off several times a year to prevent build-up.) Furniture polish can also help hide fine scratches in the surface.

Cleaning Tips

To clean the laminated surface, use a damp cloth or sponge and a mild soap or detergent. Difficult stains such as coffee or tea can be removed using a mild household cleaner and baking soda, mixed to a paste-like consistency. Using a stiff nylon bristle brush, scrub (approx. 15 to 20 strokes) the affected area. Do not scrub so hard as to mar the surface finish.

Stubborn stains that resist the above cleaning method may require the use of undiluted household bleach or nail polish remover. Using a cotton ball saturated with bleach or nail polish remover (acetone), gently rub the stain for up to two minutes. Rinse thoroughly with warm water and wipe dry using a soft cloth. This step may be repeated if the stain appears to be going away, and the color of the laminate has not been affected.

Substances to Avoid

Acidic or abrasive cleaners can damage laminate surfaces - do not use them. Drain cleaners containing lye will permanently damage the laminate surface. If you spill or splash a drain cleaner on the laminate, wipe it up immediately and rinse several times with water.

CAUTION: Prolonged exposure of the laminate surface to bleach will cause discoloration. Always rinse laminate surfaces after cleaning! Failure to rinse after cleaning can cause damage even if only a small amount of cleaning solution remains on the surface. A dry residue may be invisible, however, moisture from cups or drinks can reactivate it, and result in permanently etched scars or stains over time.

Hair, textile, and food dyes can cause permanent stains. If dye should happen to spill or splash on the laminate, wipe it up immediately with dishwashing detergent or an all-purpose cleaner. Wipe spills away promptly and rinse several times with water.

Rust removers contain harsh chemicals which will quickly cause permanent damage. If a spill or splash occurs, wipe off all residue immediately, wash thoroughly with soapy water, and rinse several times.

Steel wool and other abrasive pads will damage the laminate surface. Do not use them for cleaning, and do not leave steel wool pads on the laminate; the metal can rust and leave stains.

Toilet bowl cleaners contain harsh chemicals that can cause permanent damage. If spills or splashes occur, wipe up immediately, wash the surface with soapy water and rinse several times.

Recommended Cleaners

The following commercially available cleaners can be used on the laminated surface:

- Clorox® (avoid prolonged exposure)
- Formula 409®
- Dawn®
- Glass Plus®
- Dow Bathroom Cleaner with Scrubbing Bubbles™
- Fantastik®
- Favor®
- Windex®
- Lestoil®
- Pledge®
- Grease Relief®
- Lysol® Brand Disinfectant Basin/Tub/Tile Cleaner
- Mr. Clean®
- TOP JOB®

Cleaners to Avoid

DO NOT use the following cleaners on the laminate:

Chemical Ingredient	Synonymous Names
■ Hydrochloric Acid	<i>Muriatic Acid</i> <i>Hydrogen Chloride</i> <i>Oleic Acid</i> <i>Oil of Vitriol</i> <i>Oleum</i>
■ Hydrofluoric Acid	<i>Rust Remover</i>
■ Phosphoric Acid	<i>Rust Remover</i>
■ Sodium Hydroxide	<i>Caustic Soda</i> <i>Caustic</i> <i>Lye</i> <i>Soda Lye</i>
■ Pumice (abrasive)	

Cleaning Stainless Steel Tubs

Rinse the stainless steel tub with clear water and dry thoroughly with clean, soft cloths.

Ordinary deposits of waste and fluids can usually be removed with soap and water. Stubborn deposits may require scrubbing with “stainless steel” wool, nylon or plastic scrubbers and/or the use of commercial cleaning products. Always scrub in the direction of the “grain” of the metal. Rinse with clear water and dry thoroughly with clean, soft cloths.

Minor scale build-up and some hard water spotting may be removed by washing with vinegar, followed by a neutralizing rinse of clear water and a thorough drying with clean, soft cloths.

For heavy deposits of scale, 5% oxalic acid (use warm), 5-15% sulfamic acid, or 5-10% phosphoric acid may be used. As always, rinse with clear water and dry thoroughly with clean soft cloths.

Avoid prolonged use of chlorides (such as chlorine bleach), bromides, iodides, and thiocyanates. Never allow salty solutions to dry on the stainless steel.

Refer to *Care and Cleaning of Stainless Steel* on Page 7 for more detailed information.

Chapter 4 - Parts Replacement

Replacement Parts

The table below lists replacement parts available for the Imperial 6 Prep-Procedure Table. For parts not listed, contact SSCI Customer Service at (800) 323-7366. To order, refer to *Parts Ordering Procedure* on Page 24.

Description	SSCI Part Number	Quantity	Replacement Instructions
Door, Hinged Left or Hinged Right	Contact SSCI	0, 1, or 2, depending on table configuration	Page 25
Door Hinge	851910	2 per Swinging Door	Page 26
Door Hinge Mounting Plate	851912	1 per Hinge	Page 27
Door Hinge <i>Suburban Surgical</i> Logo Cap	854613	1 per Hinge	Page 28
Drawer	Contact SSCI	0, 3, or 4 depending on table configuration	Page 29
Drop-in Tub	48" Tables - 18180-00-HJAUDR 60" Tables - 18180-00-JFAUDR	1	Page 30
Flat Prep-Procedure Rack	48" Tables - 12950-00-HJAADR 60" Tables - 12950-00-JFAADR	1	Page 31
"V" Prep-Procedure Rack	48" Tables - 12955-00-HJAADR 60" Tables - 12955-00-JFAADR	1	Page 31
Extension Rack for Faucet Area	Flat Racks - 12950-00-BWAADR "V" Racks - 12955-00-BWAADR	1	Page 31
Solid Removable Top	48" Tables - 12960-00-HJAADR 60" Tables - 12960-00-JFAADR	1	Page 31
Removable Bathing Rack (Optional)	Stainless Steel, 48" - 12965-00-GHAFDG Stainless Steel, 60" - 12965-00-IDAFDG Plastisol Coated, 48" - 12970-00-GHAFDG Plastisol Coated, 60" - 12970-00-IDAFDG	1	Page 32

Replacement Parts - Imperial Laminated Prep-Procedure Tables

General Information

- During disassembly, retain all hardware items such as screws, nuts, lockwashers, etc. for reassembly.
- If you have problems with any procedure, please feel to call SSCI Customer Service at (800) 323-7366.

Parts Ordering Procedure

Order new equipment, accessories, and/or replacement parts directly through SSCI Customer Service. You can order by mail, telephone, or fax. Refer to *SSCI Contact Information* on *Page 6* for address, telephone, and fax numbers. When ordering parts, please provide the following information:

- Your name
- Company name
- Company account number
- Telephone number
- Fax number
- e-mail address
- Shipping address
- Billing address (if different from shipping address)
- Names, part numbers, and quantities of items being ordered
- Credit card number and expiration date, or other payment information
- Preferred method of shipment
- Information on whether the items are required on a normal or urgent basis

Returning the Prep-Procedure Table for Repairs

RMA Numbers

If your prep-procedure table should require return to SSCI for repairs, discuss the problem with one of our Customer Service Representatives. Obtain an RMA number (Return Merchandise Authorization) from them before shipping the unit back.

Note: SSCI will *not* accept merchandise returned without an RMA number.

Packing and Shipment

If you were able to keep the table shipping carton, repack the table into the carton and staple or tape the cover securely in place.

If the shipping carton is not available, package the table securely in a suitable container. Ship documentation with the table including:

- Destination
- RMA Number
- Your name, company, and address
- Your telephone number
- A description of the reason for returning the table

Parts Replacement Procedures

The following sections guide you in replacing worn, damaged, or missing parts on an SSCI Imperial 6 Prep-Procedure Table.

Door, Hinged Left or Hinged Right Contact SSCI for Part Numbers

Overview

The following instructions guide you in replacing a door hinged either left or right. For detailed information on the operation of the hinges, refer to *Page 16*.

Tool Required

- Phillips screwdriver

Procedure

1. Squeeze on the release catches of both hinges (Figure 14), and remove the door from the table. Refer to *Removing a Door* on *Page 16*.
2. With a Phillips screwdriver, remove the two screws on each hinge and remove both hinges from the old door (Figure 15).
3. With the screws removed above, mount the hinges on the new door.
4. Mount the door in the cabinet - engage the hinges into the hinge mounting plates, and snap the hinges into place. Refer to *Installing a Door* on *Page 17*.
5. Observe how the door fits in the cabinet. If necessary, adjust the door; refer to *Adjusting the Door Left-to-Right* on *Page 17* and *Adjusting the Door In-and-Out* on *Page 18*.

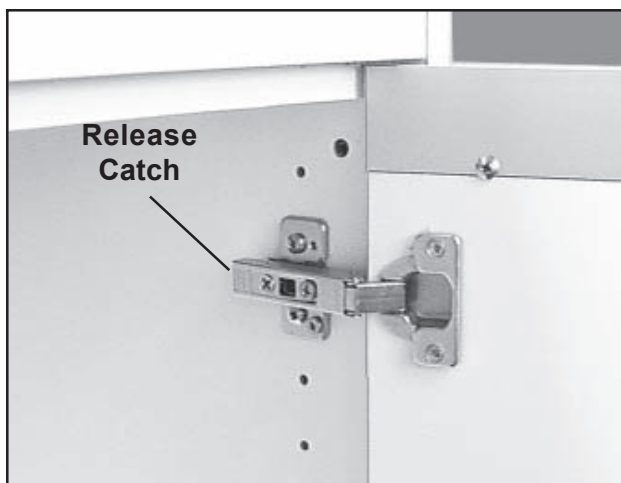


Figure 14. Door Hinge Release Catch

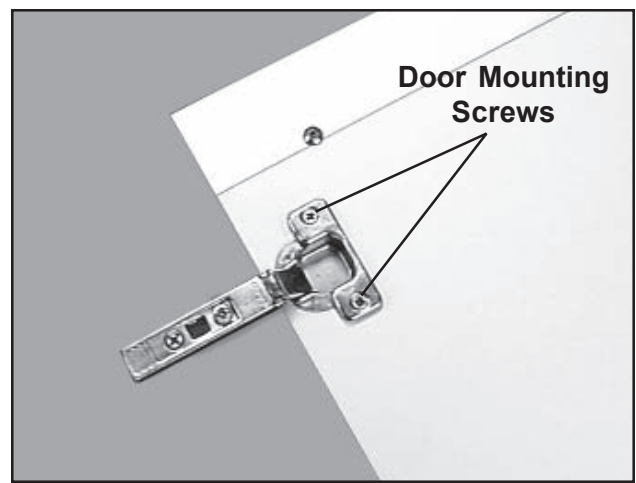


Figure 15. Hinge Mounted on Door

Door Hinge P/N 851910

Overview

The following instructions guide you in replacing a door hinge. All door hinges are identical whether the door is hinged-left or hinged-right. For detailed information on the operation of the hinges, refer to *Page 16*.

Tool Required

- Phillips screwdriver

Procedure

1. Open the cabinet door.
2. Squeeze on the release catches of both hinges (Figure 14), and remove the door from the cabinet. Refer to *Removing a Door on Page 16*.
3. With a Phillips screwdriver, remove the two mounting screws on the hinge and remove the hinge from the door (Figure 15).
4. Pull the *Suburban Surgical* logo cap off the hinge.
5. Using the two screws removed above, mount the new hinge to the door.
6. Snap the *Suburban Surgical* logo cap onto the new hinge.
7. Mount the door in the cabinet - engage the hinges into the hinge mounting plates, and snap the hinges into place. Refer to *Installing a Door on Page 17*.
8. Observe how the door fits in the cabinet. If necessary, adjust the door; refer to *Adjusting the Door Left-to-Right on Page 17* and *Adjusting the Door In-and-Out on Page 18*.

Door Hinge Mounting Plate

P/N 851912

Overview

The following instructions guide you in replacing a door hinge mounting plate. There is one mounting plate behind each door hinge. All door hinge mounting plates are identical. For detailed information on the operation of the hinges, refer to *Page 16*.

Tools Required

- Phillips screwdriver
- Pliers

Procedure

1. Open the cabinet door.
2. Squeeze on the release catches of both hinges (Figure 14), and remove the door from the cabinet. Refer to *Removing a Door* on *Page 16*.

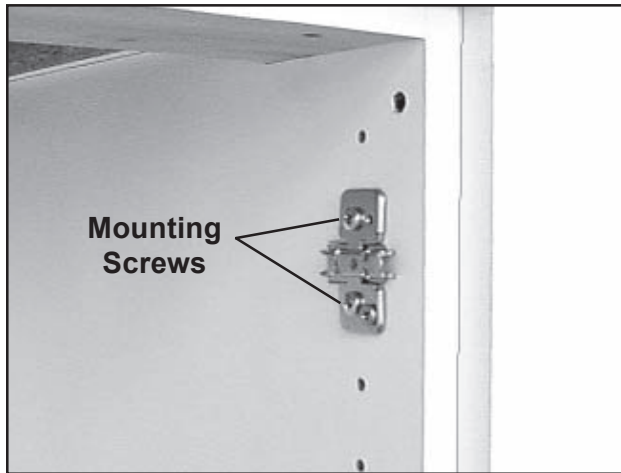


Figure 16. Door Hinge Mounting Plate

3. With a Phillips screwdriver, remove the two screws on the hinge mounting plate and remove the plate from the cabinet wall (Figure 16).
4. On the new mounting plate, two white plastic thread guards protect the plate mounting screws. Hold each guard with a pliers and, with a Phillips screwdriver, undo the screws. Discard the guards.
5. Mount the new mounting plate to the cabinet wall using the new screws supplied with the plate.
6. Mount the door in the cabinet - engage the hinges into the hinge mounting plates, and snap the hinges into place. Refer to *Installing a Door* on *Page 17*.
7. Observe how the door fits in the cabinet. If necessary, adjust the door; refer to *Adjusting the Door Left-to-Right* on *Page 17* and *Adjusting the Door In-and-Out* on *Page 18*.

**Door Hinge
Suburban Surgical
Logo Cap
P/N 854613**

Overview

The following instructions guide you in replacing a *Suburban Surgical* logo cap on a door hinge. The cap protects the door adjustment screws on the hinge from inadvertent tampering. There is one cap on each door hinge.

Procedure

1. Open the cabinet door.
2. Pull the old *Suburban Surgical* logo cap off the hinge.
3. Snap the new *Suburban Surgical* logo cap onto the hinge.

**Drawer
Contact SSCI for
Part Numbers**

Overview

The following instructions guide you in replacing a drawer. They are appropriate for both three and four drawer tables.

Procedure

1. Remove all items from the drawer.
2. Pull the drawer out, then tilt the front of the drawer up, and pull the drawer out of the cabinet.
3. To replace the drawer, slide the rollers at the rear of the drawer (Figure 18) over the rollers on the cabinet wall (Figure 19), then gently push the drawer in.

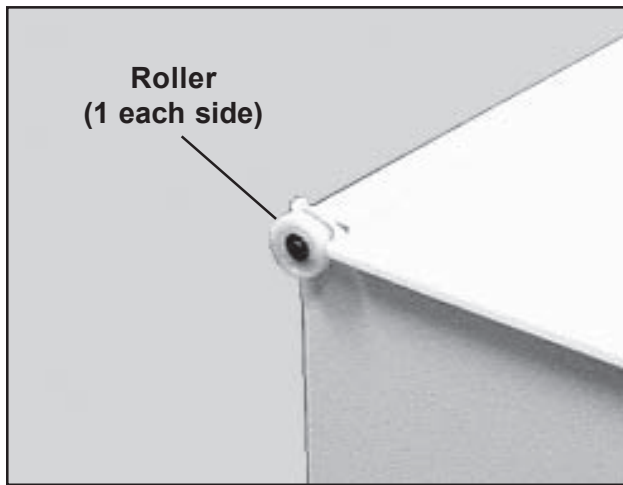


Figure 17. Roller on Rear of Drawer.

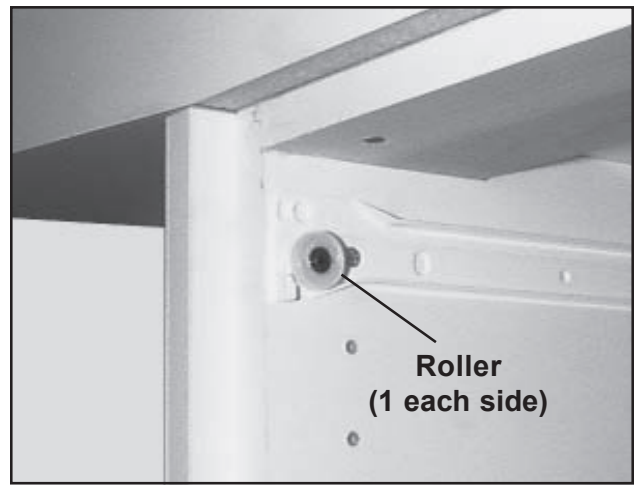


Figure 18. Roller on Cabinet Wall

Drop-in Tub

Refer to Table on *Page 23*
for Part Numbers

Overview

The following instructions guide you in replacing a drop-in tub.

Tools Required

- Plumbing tools as necessary

Procedure

CAUTION: Removing and installing a drop-in tub is not difficult. The tub is heavy, however, and handling it can be awkward for one person. We recommend that removal and installation of a drop-in tub be done by at least two people.

1. Remove any prep-procedure rack that may be on the table.
2. Remove the basket strainer from the drain opening.
3. Disconnect and remove the faucets, sprayer, and drain from the drop-in tub.
4. Lift the drop-in tub off (Figure 19). Be careful, it's a tight fit!
5. Place the new drop-in tub onto the table.
6. Reconnect the drain, faucets, and sprayer.
7. Replace the basket strainer and prep-procedure rack.



Figure 19. Drop-in Tub in Prep-Procedure Table



Figure 20. Drop-in Tub

Prep-Procedure Rack

Refer to Table on *Page 23*
for Part Numbers

Overview

The following instructions apply to all types of prep-procedure racks for the Imperial 6 Prep-Procedure table.

Procedure

CAUTION: Removing and installing a rack is not difficult. The rack is heavy, however, and handling it can be awkward for one person. We recommend that removal and installation of a rack be done by at least two people.

To remove a rack, simply pick it up by hand and lift it off the table (Figure 21). To install a rack, merely set it in place on the table.

Note: If the rack does not seem to fit, rotate it 180° and try again.

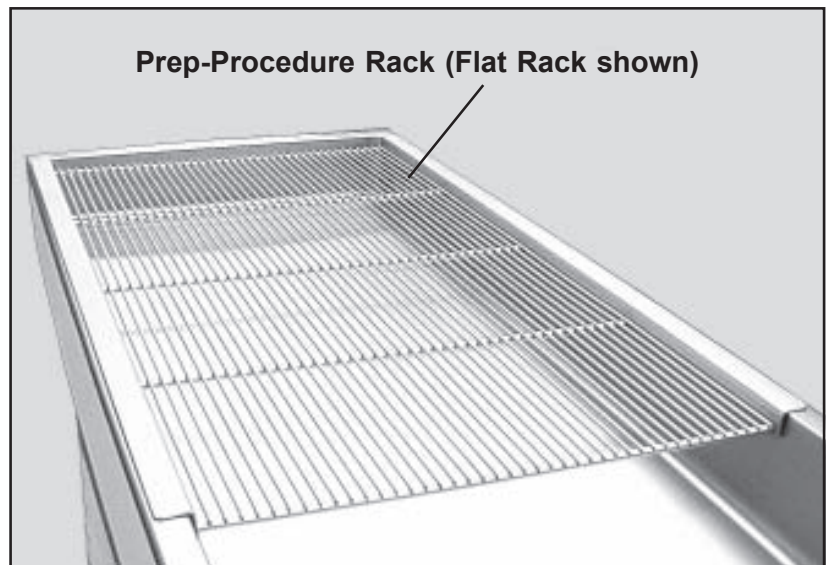


Figure 21. Prep-Procedure Rack

Removable Bathing Rack (Optional)

Refer to Table on *Page 23*
for Part Numbers

Overview

The following instructions apply to both stainless steel and plastisol coated removable bathing racks for the Imperial Prep-Procedure table.

Procedure

CAUTION: Removing and installing a rack is not difficult. The rack is heavy, however, and handling it can be awkward for one person. We recommend that removal and installation of a rack be done by at least two people.

To remove a rack, simply pick it up by hand and lift it out of the tub (Figure 22). To install a rack, merely set it in place in the tub.


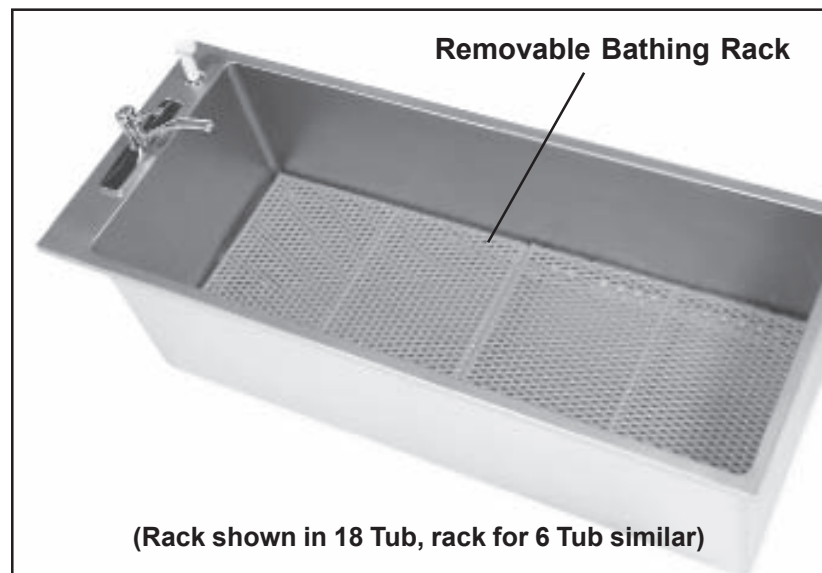


Figure 22. Removable Bathing Rack in Drop-in Tub

***For more information on SSCI's fine line of products
and accessories, talk to your SSCI sales representative.***



SSCI

Suburban Surgical Company, Inc.

275 Twelfth Street

Phone: (847) 537-9320

Toll Free: (800) 323-7366

Wheeling, IL 60090

Fax: (847) 537-9061

Web: www.suburbansurgical.com